



HAL
open science

Light emitting devices and integrated electrochemical sensors on lab-on-chip for toxicity bioassays based on algal physiology

Aliki Tsopela, Adrian Laborde, Ludovic Salvagnac, Isabelle Séguy, Ricardo Izquierdo, Philippe Juneau, Pierre Temple-Boyer, Jérôme Launay

► To cite this version:

Aliki Tsopela, Adrian Laborde, Ludovic Salvagnac, Isabelle Séguy, Ricardo Izquierdo, et al.. Light emitting devices and integrated electrochemical sensors on lab-on-chip for toxicity bioassays based on algal physiology. 18th international conference on solid-state sensors, actuators and microsystems (TRANSDUCERS 2015), Jun 2015, Anchorage, AK, United States. 4p., 10.1109/TRANSDUCERS.2015.7181251 . hal-01874764

HAL Id: hal-01874764

<https://laas.hal.science/hal-01874764v1>

Submitted on 14 Sep 2018

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

LIGHT EMITTING DEVICES AND INTEGRATED ELECTROCHEMICAL SENSORS ON LAB-ON-CHIP FOR TOXICITY BIOASSAYS BASED ON ALGAL PHYSIOLOGY

A. Tsopela^{1,2}, A. Laborde^{1,2}, L. Salvagnac^{1,2}, I. Séguy^{1,2},
R. Izquierdo³, P. Juneau³, P. Temple-Boyer^{1,2}, J. Launay^{1,2}

¹LAAS-CNRS; 7 avenue du colonel Roche, F-31400 Toulouse, France

²Université de Toulouse; UPS; LAAS; F-31400 Toulouse, France

³Université du Québec à Montréal; 201 Président Kennedy; Montréal, Canada

ABSTRACT

In the frame of water toxicity analysis, a portable, glass-based, lab-on-chip was developed, integrating three-electrode electrochemical microsensors and organic light-emitting diodes (OLED). The basic detection principle consists in monitoring electrochemically O₂-related, algal metabolism in presence of herbicides. Thus, aiming on Diuron herbicide detection, a concentration-dependent inhibition effect on photosynthetic oxygen production rate was evidenced in the [0 – 1 μM] range. Finally, OLED-based integrated system demonstrates higher detection characteristics than those using external white light source (sensitivity: 0.48 versus 0.26 nA/s/μM) and is highly promising for further integration of optical and electrochemical sensors enabling double complementary detection.

KEYWORDS

Lab-on-chip, microelectrode, OLED, O₂-related algal metabolism, herbicide detection, water toxicity analysis

INTRODUCTION

Assessment of water quality has become an increasingly important environmental issue in the past few years. Water pollution induced by agricultural and industrial activities is known to have a severe impact on all living organisms. This is associated to the excessive use of herbicides and pesticides to protect crops. These toxicants can easily penetrate the soil and are finally detected in ground and/or river waters. It is therefore a major challenge to monitor their different quantities. Although water toxicant detection is most commonly performed in laboratories, it is important to find alternative methods to existing analysis tools, more adapted to field detection. Biosensors and bioassays can eventually meet the implemented requirements and have attracted wide attention [1]. For instance, optical [2] and electrochemical [3] algal-based systems are proposed in literature for the detection of herbicides as their metabolism is highly influenced by such toxic species.

In this study, a portable, glass-based, lab-on-chip was developed to monitor algal metabolism and detect targeted herbicides. It involves three-electrode (Pt – Pt – Ag/AgCl) electrochemical microcells (ElecCell) to perform electrochemical analysis, as well as organic light-emitting diodes (OLED) to trigger algal photosynthetic activities.

EXPERIMENTAL

Electrochemical microcells (ElecCell) and organic light-emitting diodes OLED were assembled on a lab-on-chip. Six independent detection chambers were designed on each platform enabling simultaneous processing of different assays. Three fluidic chambers were dedicated to electrochemical detection and three to future fluorescence-based optical detection. The lab-on-chip structure was fabricated on glass substrate in order to be compatible with optical technology and associated measurement.

Fabrication procedure included electrochemical microcell integration on the glass substrate, fluidic microsystem implementation, and device packaging. A 3D model of lab-on-chip sensor platform, including 6 independent chambers is presented in Figure 1.

Required parameters are missing or incorrect.

Figure 1: 3D model of the lab-on-chip sensor platform.

Integration of electrochemical microcells

Concentric, three-electrode (Pt – Pt – Ag/AgCl) electrochemical microcells (ElecCell) were integrated on glass substrate through photolithography patterning and physical vapor deposition (PVD) according to a previously developed process [4,5]. Three PVD steps were performed in a row. First, a 200nm platinum layer was deposited on a 20nm titanium underlayer to form platinum-based working and counter microelectrodes. Then, a 400nm silver layer was deposited on top and was later oxidized in chloride-based solutions to form the integrated Ag/AgCl pseudo-reference microelectrode. Finally, a Si₃N₄ passivation layer, deposited by chemical vapor deposition (CVD), was patterned in order to insulate electrically the different microelectrodes and define precisely their active surface. To improve detection properties, specific attention was brought on working microelectrode design and functionalization. Thus, a microelectrode array involving 25 disks of 10μm diameter was realized and later functionalized thanks to a black platinum (BI-Pt) electrodeposition process.

Implementation of the fluidic microsystem and device packaging

The fluidic microsystem was structured by patterning 250μm-thick SU8 photoresist. Dimensions were specified according to the ElecCell geometry as well as to requirements related to the optical system. Consequently, circular-shaped fluidic analysis microchambers were

designed with a 8mm diameter and therefore a 12.5 μ L volume. Finally, the fluidic platform was sealed by wafer bonding using a glass cover. Finally, device packaging and electrical connection were performed in order to obtain a plug-in, easy to use, lab-on-chip device for algal solution analysis (Fig. 2).

Required parameters are missing or incorrect.

Figure 2: Algal test solution inserted in one of the detection chambers of the lab-on-chip device.

Bioassays and electrochemical analysis of algal photosynthetic activities

Chlamydomonas reinhardtii green algae were cultivated at 25°C in high salt medium (HSM) thanks to time-regulated light/dark (16h/8h) cycles. Algal cell concentration was measured by a multisizer Coulter counter in order to ensure a constant value for the different experiments. After leaving algae in dark for a sufficiently long time period, herbicide detection tests were finally conducted by mixing algal solutions with different Diuron concentrations (range: 0 – 1 μ M, in agreement with maximum acceptable value implied in Canada: 0.64 μ m). Using the (Pt/Bi-Pt – Pt – Ag/AgCl) ElecCell, O₂ monitoring was finally performed by chronoamperometry with an applied potential of -0.7 V versus integrated Ag/AgCl. All the experiments were performed at ambient temperature (~ 22°C).

Thanks to its realization on a glass substrate, the glass-based lab-on-chip was fully compatible with optical technology and associated measurement (Fig. 2). As a result, it allowed herbicide detection while using a non-integrated, halogen, white light source. However, in order to eventually obtain portable and autonomous analysis microsystem, the light source used for the stimulation of algal photosynthetic activities should be integrated on the final lab-on-chip device. Consequently, blue OLED devices were fabricated on a glass substrate through multilayer evaporation of PEDOT:PSS/NPB/PCAN/Alq₃/Al and placed on top of the detection chamber, in direct contact with the lab-on-chip glass cover (Fig. 3). It was specifically designed in order to have a good overlap between the OLED electroluminescence spectrum and the *Chlamydomonas reinhardtii* algae absorption band (Fig. 4).

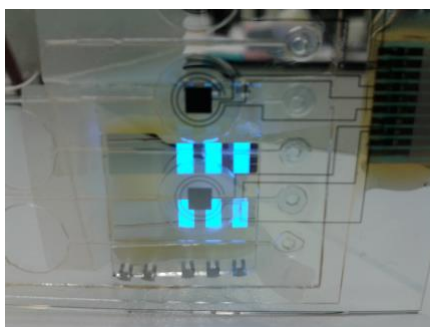


Figure 3: Integration of blue OLED devices on the lab-on-chip glass cover.

Required parameters are missing or incorrect.

Figure 4: Comparison of emission spectra of OLED and halogen white light source with algal absorption spectrum.

RESULTS AND DISCUSSION

O₂ measurement in control algal solutions

Using the halogen white light source, dark and light periods were alternated in control algal solutions and O₂ concentration was monitored by chronoamperometry (Fig. 5). When light is on, photosynthesis is responsible for oxygen production and therefore for the O₂-related cathodic reduction current increase. On the contrary, when light is off, algae are consuming oxygen due to respiration and the cathodic reduction current decreases. Prior to further analysis, it was checked, using non-algal control solutions that current variations were not related to illumination interferences (result not shown).

Thanks to these first experiments, it appeared that current follows roughly linear variations with time and therefore that algal metabolisms can be studied according to the slope of the current versus time.

Furthermore, a compromise was found concerning algal concentration in order to yield well-defined differences between oxygen production and consumption and high signal-to-noise ratio. This leads to an optimal concentration around 13 \times 10⁶ cells/mL. This value was chosen for the following experimental campaigns.

Required parameters are missing or incorrect.

Figure 5: Current measurements of algal respiration and photosynthesis using a (Pt/Bi-Pt – Pt – Ag/AgCl) ElecCell device integrated on a lab-on-chip.

Diuron detection using halogen white light source

First experiments were performed using a halogen white source illumination. Light-induced oxygen production was monitored in real time and O₂ production rate decrease with increasing Diuron concentration points out the toxicant effect (Fig. 6). Nevertheless, respiration rates before turning on the light were found to be not identical. Since Diuron herbicide targets only photosynthetic activity, the causes of this variability are difficult to determine. They can be related to algae culture intrinsic properties, sampling protocol and/or biofouling phenomena.

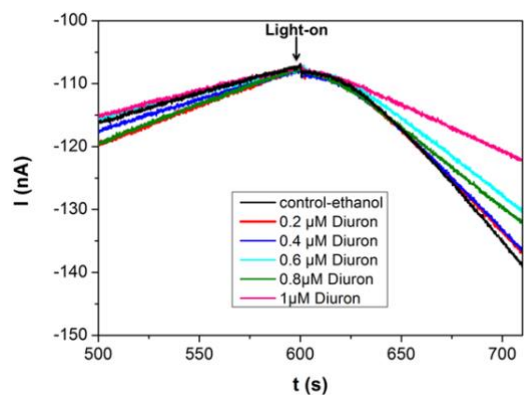


Figure 6: Algal O_2 -amperometric responses for various Diuron concentrations using a (Pt/Pt-BI - Pt - Ag/AgCl) ElecCell-based lab-on-chip device.

As a result, a normalization step was conducted in order to eliminate this variability. It consists in setting an average "reference" value \bar{x} for the different respiration slopes (x_i) and applying a correction coefficient to all the photosynthesis slopes (y_i).

$$y_i^* = y_i \frac{\bar{x}}{x_i} \quad (1)$$

Through this approach, sensor calibration curves were defined by studying the photosynthetic O_2 production rate for different Diuron concentrations (Fig. 7). For the two light intensities tested, a linear decrease was obtained between both parameters, allowing to define the Diuron detection sensitivity. Values of 0.26 and 0.1 nA/s/ μ M were calculated for light intensities of 600 and 1800 μ E/m²/s respectively.

Required parameters are missing or incorrect.

Figure 7: Calibration curves (normalized oxygen production rates versus Diuron concentration) for two different light conditions using halogen white light source.

Light intensity is known to play an important role in algal metabolism. At low intensity levels, photosynthesis is enhanced when light intensity is increased as more photons are captured by pigments and processed through the chloroplast reaction centers [6]. However, at high intensity levels, reaction centers of chloroplast become saturated or even damaged. An inhibition of photosynthetic activity is thus observed [7]. Our result demonstrates that, when illumination conditions are too high, they are responsible for such inhibition phenomenon.

Finally, it should be noted that herbicide detection was also performed using natural lake water to cope with real samples analysis. Thus, Diuron detection sensitivity around 0.26 nA/s/ μ M was still obtained for a 600 μ E/m²/s light

intensity (Fig. 8).

Diuron detection using blue OLED as light source

Given the fact that blue OLED devices were integrated on the ElecCell-based lab-on-chip at the system level, a non-algal control measurement of current monitoring through light/dark periods was conducted. In contrast with previous control measurement carried out with the non-integrated halogen white light source, an increase in the cathodic reduction current was observed when the light was turned on (result not shown). This current increase was attributed to the temperature increase induced by OLED heating. Indeed, the temperature on the lab-on-chip backside was measured around 35°C after a two minutes blue OLED illumination. In order to compensate this phenomenon, the illumination rate recorded for the non-algal control solution was subtracted from the photosynthetic O_2 production rate determined for different Diuron concentrations. Experiments were performed in natural lake water samples in the [0 - 0.6 μ M] Diuron concentration range (Fig. 8). Detection sensitivity obtained when using the integrated blue OLED light source was estimated at around 0.48 nA/s/ μ M that corresponds to almost double the value obtained while using the non-integrated halogen white light source. This sensitivity improvement was related to the better overlap between the blue OLED emission spectrum with the major *Chlamydomonas reinhardtii* algae absorption band (Fig. 4).

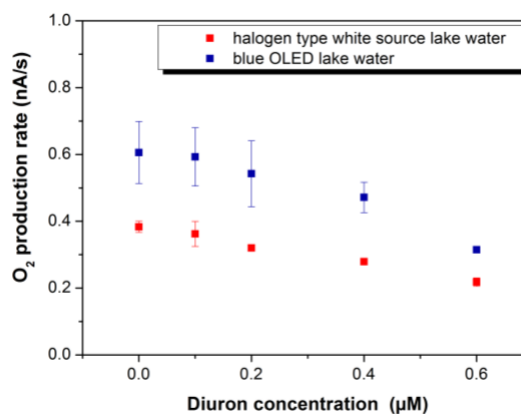


Figure 8: Calibration curves obtained in lake water samples using as light sources, either an integrated blue OLED (blue points) or a halogen white light source (red points).

CONCLUSION

A portable device for in-situ herbicide detection, based on algal physiology, was developed. The fabricated lab-on-chip platform consists in three fluidic chambers integrating (Pt/Bi-Pt - Pt - Ag/AgCl) electrochemical microcells (ElecCell) and three chambers dedicated to further optical fluorescence-based detection. The effect of Diuron herbicide was validated using the lab-on-chip devices with culture medium solutions. Illumination was first supplied through a

non-integrated, halogen white light source. Thus, a Diuron concentration-dependent decrease in the photosynthetic oxygen production rate was demonstrated for two different light intensities: 600 and 1800 $\mu\text{E}/\text{m}^2/\text{s}$. Diuron detection sensitivity of approximately 0.26 and 0.1 nA/s/ μM were respectively obtained, evidencing photosynthesis inhibition phenomena due to too high intensity levels. Then, in order to obtain an autonomous system, the same experiments were successfully carried out in natural lake water samples, with an integrated blue OLED used as light source for the excitation of photosynthetic mechanism. Taking into account undesired heating phenomena, Diuron detection was found to gain a factor two (value around 0.48 nA/s/ μM in the [0 – 0.6 μM] concentration range) evidencing that photosynthetic apparatus was more effective when the blue OLED light source is used compared to the halogen white light source.

These first results demonstrate that the proposed lab-on-chip biosensor can effectively follow the change in photosynthetic activity induced by Diuron herbicide and reflected through a modification in oxygen production rate. It can therefore be an efficient indicator of water pollution. Nevertheless, further studies should be conducted to still improve detection properties while optimizing the OLED photoluminescence spectrum, illumination power and integration process.

ACKNOWLEDGEMENTS

The authors would like to thank the French "Agence nationale de la Recherche" (ANR, project DOLFIN, n° ANR-13-JS03-0005-01) and the "Fonds France Canada pour la Recherche" (FFCR) for financial support. Finally, microfabrication procedure was partly supported by the French RENATECH network.

REFERENCES

- [1] A. Jang, Z. Zou, K.K. Lee, C.H. Ahn, P.L. Bishop, "State-of-the-art lab chip sensors for environmental water monitoring", *J. Measurement Science & Technology*, 032001 (18pp), 2011.
- [2] F. Lefèvre, A. Chalifour, L. Yu, V. Chodavarapu, P. Juneau, R. Izquierdo "Algal fluorescence sensor integrated into a microfluidic chip for water pollutant detection", *Lab chip*, vol. 12, pp. 787-793, 2012.
- [3] I. Shitanda, S. Takamatsu, K. Watanabe, M. Itagaki, "Amperometric screen-printed algal biosensor with flow injection analysis system for detection of environmental toxic compounds", *Electrochimica Acta*, vol. 54, pp. 4933-4936, 2009.
- [4] S. Ben Amor, E. Vanhove, F. Sékli Belaïdi, S. Charlot, D. Colin, M. Rigoulet, A. Devin, J. Launay, P. Temple-Boyer, S. Arbault: "Enhanced detection of hydrogen peroxide with platinized microelectrode arrays for analyses of mitochondria activities", *Electrochimica Acta*, vol. 126, pp. 171-178, 2014.
- [5] A. Tsopela, A. Lale, E. Vanhove, O. Reynes, I. Séguy, P. Temple-Boyer, P. Juneau, R. Izquierdo, J. Launay:

"Integrated electrochemical biosensor based on algal metabolism for water toxicity analysis", *Biosensors and Bioelectronics*, vol. 61, pp. 290-297, 2014.

- [6] C.W. Cho, T.P.T. Pham, Y.C. Jeon, J. Min, H.Y. Jung, D.S. Lee, et Y.S. Yun: "Microalgal photosynthetic activity measurement system for rapid toxicity assessment", *Ecotoxicology*, vol. 17, pp. 455-463, 2008.
- [7] J. Barber et B. Andersson: "Too much of a good thing: light can be bad for photosynthesis", *Trends in Biochemical Sciences*, vol. 17, pp. 61-66, 1992.

CONTACT

*J. Launay, Tel: +33-561 336 809; jlaunay@laas.fr